


22/23

10  
~~Figure 3c~~ **Figure 3c** Determination of ApoC-III level in 14 haemorrhagic and 13 ischaemic stroke plasma samples compared to 30 negative controls using Daiichi tests (Cobas Mira plus automate)

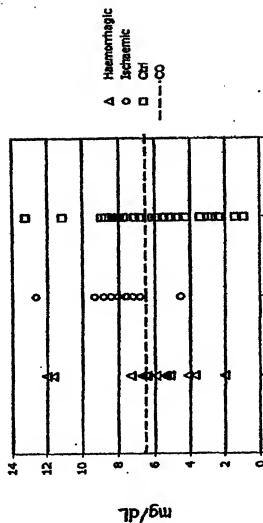

	P (student test)	Sensitivity	Specificity
I vs H	0.0342	92.3 %	71.42 %
I vs Ctrl	0.025	92.3 %	50 %
H vs Ctrl	0.4682	-	-